


HOW TO MIX

BRAVECTO[®]
injectable

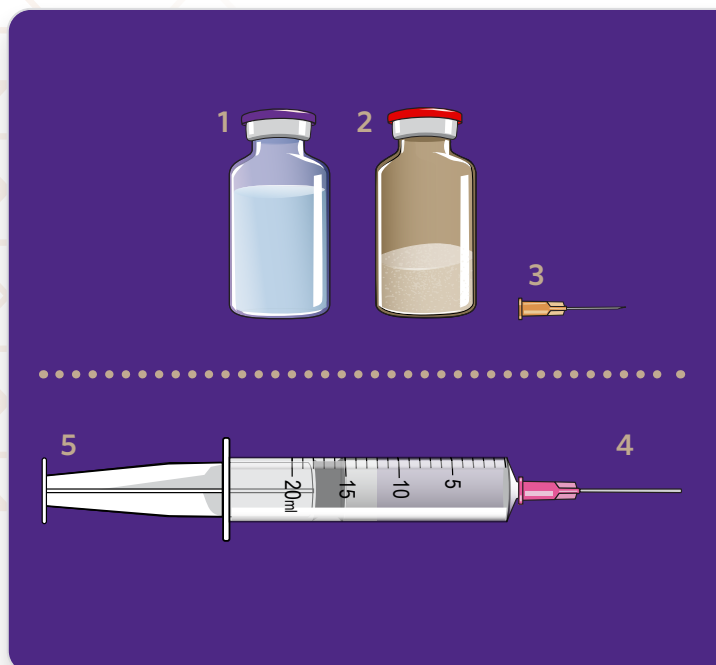

The package includes:

- Solvent vial (1)
- Fluralaner powder vial (2)
- Vent needle (25 G) (3)
- Package leaflet


You will need to provide:

- Sterile transfer needle (18 G) (4)
- Sterile 20 ml syringe for transfer (5)

To ensure effective treatment, it is important to correctly mix the suspension before injection and use the recommended syringe and needle sizes as listed under the directions in the product information.



Begin by shaking the fluralaner powder vial to break up any aggregates prior to reconstitution.

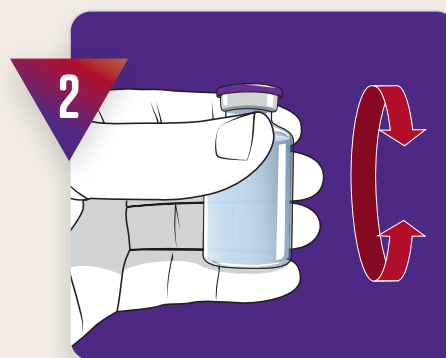


Invert the solvent vial at least 3 times until visibly uniform. The content of the solvent vial is a clear to opaque viscous solution.

Instructions continued on next page ...

HOW TO MIX BRAVECTO[®] injectable

3

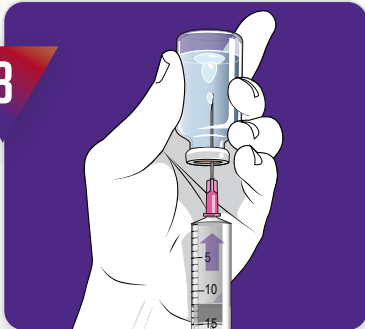


Remove the purple cap of the sterile solvent vial. Using the 18 G needle and the 20 ml syringe, inject up to 14 ml of air into the solvent vial.

Then, **withdraw 15ml ONLY** of solvent from the vial.


It is important to note that there is more solvent supplied in the vial than required for reconstitution.

4

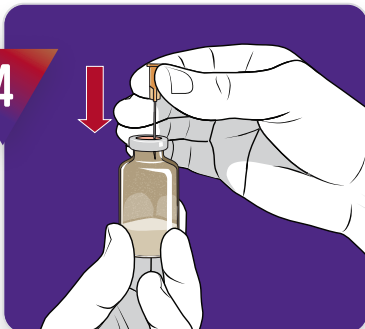


Remove the red cap of the fluralaner powder vial. **Insert a 25 gauge vent needle** into the top of this vial.

5

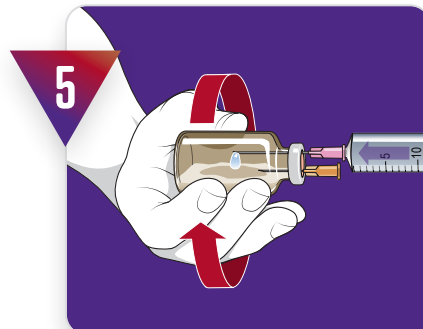

While **rotating the vial horizontally in your hand**, slowly transfer the solvent into the fluralaner powder vial to ensure complete wetting of the powder.

6

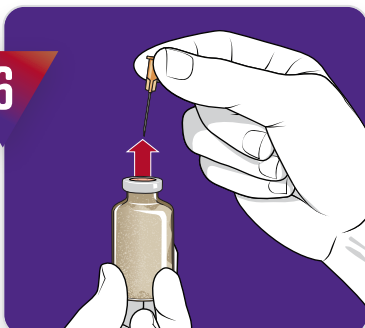

Once the solvent has been added, remove the vent and transfer needles from the fluralaner powder vial and discard the needles safely and appropriately.

7



Shake the vial vigorously for at least 30 seconds until a thoroughly mixed suspension of the fluralaner powder and solvent is produced. **Before every use, shake the reconstituted vial vigorously for at least 30 seconds to achieve a uniform suspension.**

BRAVECTO injectable may be stored below 30°C for 3 months after reconstitution. Discard the reconstituted vial after 20 punctures to the stopper or if the product has been suspended for more than 3 months.

For more details, view the mixing video at mix.bravecto.com or scan the QR code



Legal categories: RoI **POM** NI: **POM-V**

Contains fluralaner. For further information about side effects, precautions, warnings and contra-indications please consult your veterinary practitioner or the product SPC, packaging leaflets or: MSD Animal Health, Red Oak North, South County Business Park, Leopardstown, Dublin 18, Ireland. Tel: +353 (0)1 2970220. Email: vet-support.ie@msd.com Web: www.msd-animal-health.ie

USE MEDICINES RESPONSIBLY

SA-23-107 IE-BRV-231200008 FEB 2024



MSD
Animal Health